

FIGURE 1

FIG. 2 is a cross-sectional view of the device 10 in a second position, where the container 12 is inverted and the liquid 20 is being dispensed into the container 16.

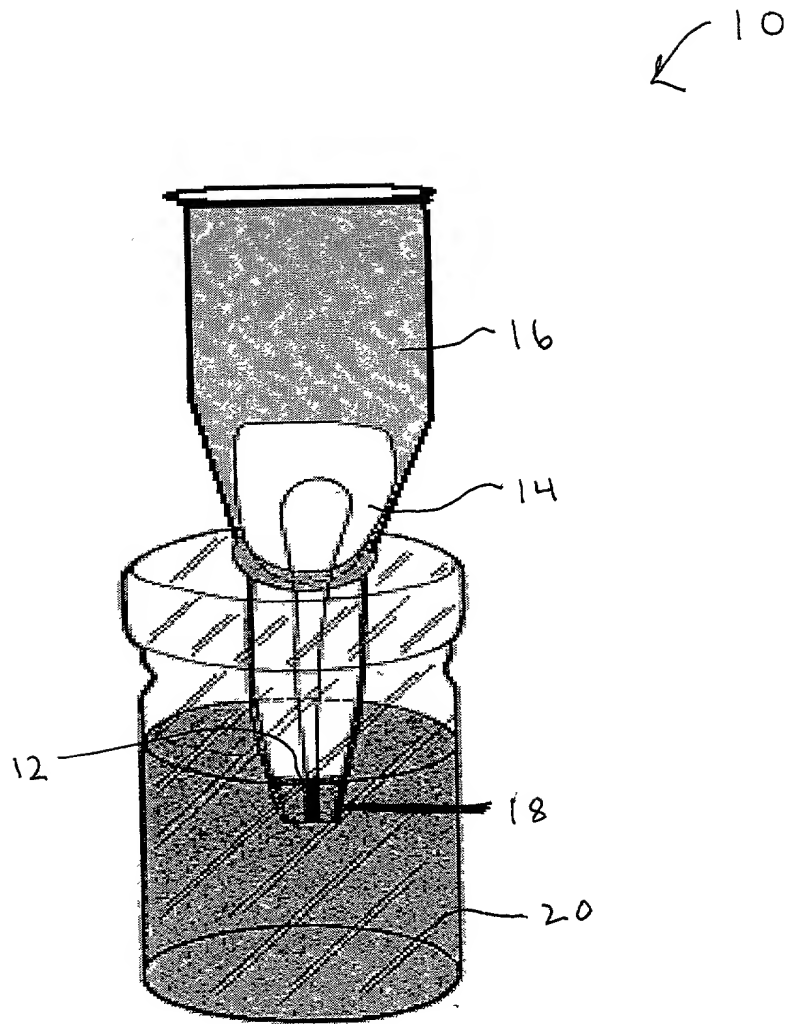


FIGURE 2